

Porcine IgG ELISA development kit

Product Code: 3151-1HD-6

CONTENTS: development kit for 6 plates

Vial 1 (green top)

Monoclonal antibody MT421 (300 μ l)

Concentration: 0.5 mg/ml

Vial 2 (yellow top)

Monoclonal antibody MT424-HRP (80 μ l)

Vial 3

Lyophilised porcine IgG standard

To ensure total recovery of stated quantity, vials have been overfilled.

STORAGE:


Shipped at ambient temperature. On arrival box 1 should be stored refrigerated at 4-8°C and box 2 should be stored frozen at -20°C.

General

Intended use: For quantitative determination of native porcine IgG in serum and plasma.

Reagents: MT421 is supplied in sterile-filtered (0.2 μm) PBS with sodium azide (0.02%). MT424-HRP is supplied in storage buffer with 0.002% Kathon.

Standard range: 0.05-25 ng/ml

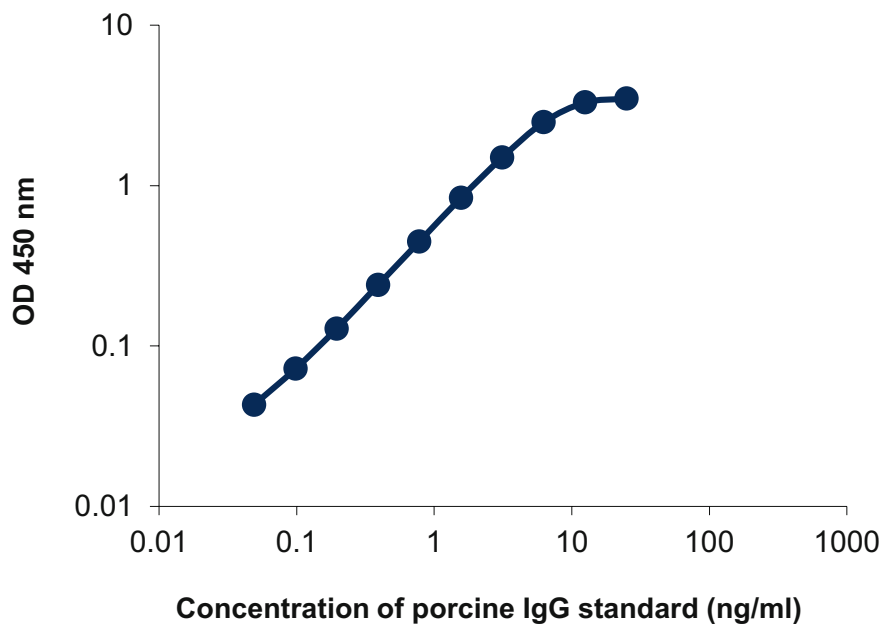

Guidelines for Porcine IgG ELISA

- Day 1** 1. Coat a high protein binding ELISA plate with MT421 antibody, diluted to 2 µg/ml in PBS, pH 7.4, by adding 100 µl/well. Incubate overnight at 4-8°C.
- Day 2** 2. Wash twice with PBS (200 µl/well).
3. Block plate by adding 200 µl/well of PBS with 0.05% Tween 20 (PBS-Tween) containing 0.1% BSA (incubation buffer*). Incubate for 1 hour at room temperature
4. Wash five times with PBS-Tween.
5. Prepare bovine IgG standard by reconstituting contents of vial 3 in 500 µl PBS to make up a stock solution of 50 µg/ml. The stock solution should be used immediately or stored in aliquots at -20°C for future use. We recommend the aliquots not be refrozen after initial use. For the test, prepare dilutions of the stock using the standard range as a guideline.
6. Add 100 µl/well of samples or standards diluted in incubation buffer. It is recommended to make serial dilutions of samples to obtain results within the standard range. Incubate for 2 hours at room temperature.
7. Wash as in step 4.
8. Add 100 µl/well of MT424-HRP diluted 1:1000 in incubation buffer. Incubate for 1 hour at room temperature. **Please note that sodium azide used in buffers will inhibit HRP activity.**
9. Wash as in step 4.
10. Add 100 µl/well of appropriate substrate solution.
11. Measure the optical density in an ELISA reader after suitable developing time. If required stop the reaction first.

* The same buffer is used for blocking and for dilution.

Developed and manufactured by MABTECH AB, Sweden, whose quality management system complies with the standards ISO 9001:2015 & ISO 13485:2016.



The products are for research use only.

MABTECH shall not be liable for the use or handling of the product or for consequential, special, indirect or incidental damages there from.

Mabtech AB (Head Office)
Sweden
Tel: +46 8 716 27 00
mabtech@mabtech.com

Mabtech, Inc.
USA
Tel: +1 513 871-4500
mabtech.usa@mabtech.com