


# ELISA PathRF: Human IFN- $\gamma$

3420-1HP-DP-1

**Datasheet & Protocol**





# Table of Contents

Introduction ..... 4

Shipping and storage ..... 4

Contents ..... 5

Preparation ..... 6

Protocol ..... 8


Performance..... 10

# Introduction

ELISA PathRF for quantification of human IFN- $\gamma$  in plasma and serum samples containing rheumatoid factor (RF). For Research Use Only (RUO). Not for use in diagnostic procedures.

## ELISA assay principle

ELISA PathRF kits are supplied with ELISA strip plates precoated with monoclonal antibody (mAb). Analyte in the sample is captured by the coated mAb and detected by the recombinant biotinylated detection mAb followed by Streptavidin-HRP (SA-HRP). Addition of TMB substrate will result in a colored substrate product. The reaction is stopped with sulfuric acid and the optical density can be quantified using an ELISA plate reader. The concentration of analyte is determined by comparison to a serial dilution of the ELISA standard analyzed in parallel.

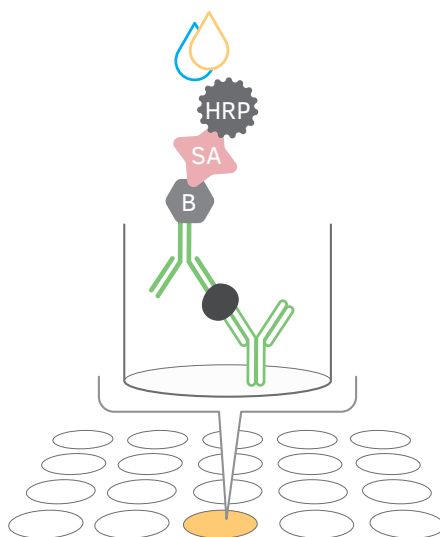

## Analysis of serum and plasma samples

ELISA PathRF kits are designed to eliminate potential interference from RF and heterophilic antibodies. The combination of a recombinant detection mAb and RF-block diluent prevents RF and heterophilic antibodies from cross-linking the assay antibodies, effectively reducing the risk of false-positive signal. RF and heterophilic antibodies can be found at high concentrations in serum and plasma from individuals with autoimmune diseases such as rheumatoid arthritis. The kit has been validated with RF-containing plasma.

## Shipping and storage

The kit is shipped at ambient temperature. All reagents should be stored at 4–8 °C upon receipt. The expiry date indicates how long unopened products, stored according to instructions, are recommended for use. Do not combine components from different kit batches or components from other suppliers.

# Contents

## Component

Pre-coated ELISA strip plate: Anti-IFN- $\gamma$ mAb 1-D1K	1 x 96 wells
Recombinant human IFN- $\gamma$ ELISA standard	1 vial
Detection mAb MTR-10, biotinylated (0.5 mg/ml)	30 $\mu$ l
Streptavidin-HRP	15 $\mu$ l
Standard reconstitution buffer A8	1 ml
Wash buffer concentrate (20x)	120 ml
RF-block diluent	60 ml
Streptavidin-HRP diluent	15 ml
TMB substrate	15 ml
Stop solution	15 ml
Adhesive plate covers	3

To ensure total recovery of the stated quantity, bottles and vials have been overfilled.

## Materials required but not supplied

- Microplate reader capable of reading at 450 nm
- ELISA plate washer; automated or manual (e.g., multipipette or squirt bottle)
- Precision pipettes, tips, and graduated cylinders
- Tubes for standard and sample dilutions
- Distilled or deionized water

## Safety information

The Stop solution, 0.18 M H<sub>2</sub>SO<sub>4</sub> (< 1%), is irritating to eyes and skin and should be handled with care. The standard should also be handled carefully as the effects of exposure are unknown. Buffers and reagents in solution contain the preservative Kathon CG (0.002%), a potential allergen that may cause sensitization through skin contact. Human and animal samples should be treated as potentially hazardous biologic material. All material should be disposed of in accordance with local regulations. For further information please consult the Safety Data Sheet on our website.

## Preparation

- Allow the plates and assay reagents to reach room temperature before starting the assay (except for the TMB substrate which should preferably be used cold).
- Plan the plate layout to include a standard curve, samples, and an assay background control, all in duplicate. The volume per well should not exceed 100 µl. Include a plate blank (wells with only Substrate and Stop solution) to be used for subtraction before analysis.

### Wash buffer

Add 50 ml Wash buffer concentrate to 950 ml distilled or deionized water (sufficient for all washing steps of 1 plate). If crystals have formed in the 20x concentrate, bring to room temperature and mix gently to dissolve.

### Samples


For accurate assay performance, all samples should be diluted at least 2-fold in RF-block diluent. Samples can be diluted in tubes or plates; diluent should be added before the samples and visible precipitates should be removed. The use of strongly hemolyzed and hyperlipemic samples may give inaccurate determination of the concentration. Samples containing high levels of analyte exceeding the standard range of the assay will require further dilution.

### ELISA standard

Reconstitute the ELISA standard to a stock solution of 0.2 µg/ml by adding 1 ml Standard reconstitution buffer. Allow the standard to dissolve for 5 minutes and mix thoroughly. The standard should be kept in aliquots at -20 °C. Avoid repeated freeze-thaw cycles.

### Preparation of standard curve

Dilute the standard stock solution to create a standard curve as shown. The indicated volumes are sufficient for duplicates. The last vial is used as an assay background control, i.e., the standard should be omitted. Prepare the standard curve within 30 minutes of use.

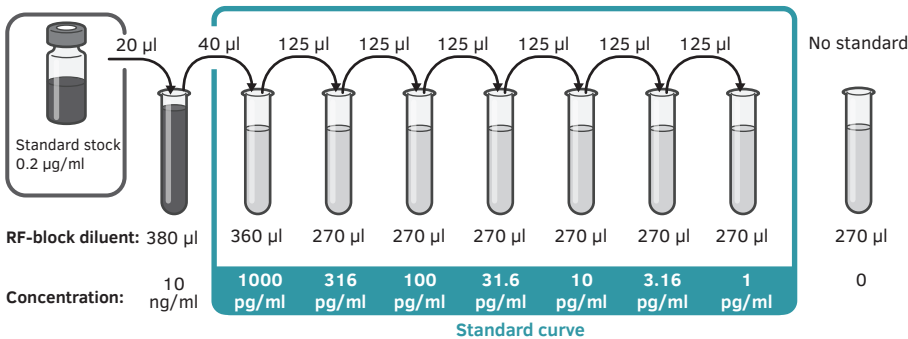

### Detection antibody

Dilute the detection mAb in RF-block diluent to 1 µg/ml within 15 minutes of use. For each plate, add 24 µl detection mAb to 12 ml RF-block diluent.

### Streptavidin-HRP

Dilute the Streptavidin-HRP 1:1000 in Streptavidin-HRP diluent within 15 minutes of use. For each plate, add 12 µl Streptavidin-HRP to 12 ml Streptavidin-HRP diluent.

# Protocol


Prepare the reagents, standard curve, and samples as described in the Preparation section. Assemble the required number of strips in the plate frame and label the top of each strip. Store the remaining strips in the foil bag containing the desiccant at 4-8 °C.

1. Wash the plate 5 times with wash buffer, 300 µl per well. After the final wash, invert and tap the plate firmly against absorbent paper. Immediately proceed to the next step.
2. Add 100 µl per well of samples (diluted at least 2-fold), standard, and assay background control. Mix by tapping the plate. Cover the plate with an adhesive plate cover and incubate for 2 hours at room temperature.
3. Wash as in step 1.
4. Add 100 µl per well of detection mAb. Cover the plate and incubate for 1 hour at room temperature.
5. Wash as in step 1.
6. Add 100 µl per well of Streptavidin-HRP. Cover the plate and incubate for 1 hour at room temperature.
7. Wash as in step 1.
8. Add 100 µl of TMB substrate to each well. Incubate at room temperature, protected from direct light for 15 minutes.
9. Add 100 µl of Stop solution to each well to stop the color development.
10. Measure absorbance at 450 nm within 15 minutes. Preferably use a reader capable of subtracting a reference wavelength between 570 and 650 nm.

We recommend the use of an ELISA software utilizing a 4- or 5-parameter curve fit. Subtract the mean absorbance value of the blank from the samples, standard and assay background control prior to creating the standard curve and analyzing the results.




Wash




Add samples,  
standard, and assay  
background control  
Incubate 2 hours

Wash




Add detection  
antibody  
Incubate 1 hour

Wash




Add Streptavidin-HRP  
Incubate 1 hour


Wash



Add TMB substrate  
Incubate 15 minutes



Add Stop solution




+



Measure absorbance  
at 450 nm within  
15 minutes

# Performance

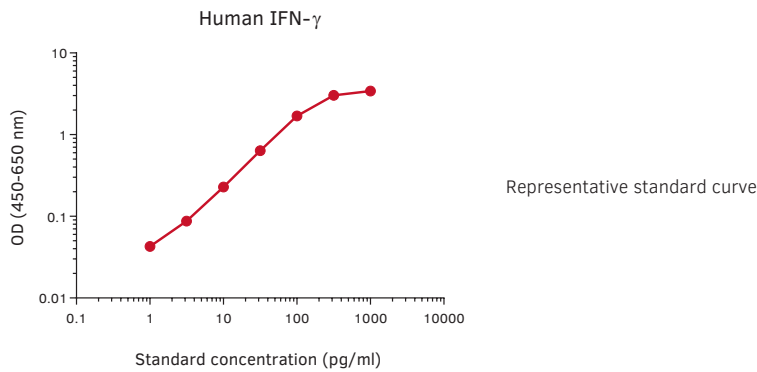

**Standard range** 1-1000 pg/ml

**Sensitivity** 0.6 pg/ml

The lowest concentration that can be detected, but not necessarily quantified with precision and accuracy. This was determined by adding 4 standard deviations to the mean OD of background wells.

## Calibration

The standard of this ELISA has been calibrated against an international standard from the National Institute of Allergy and Infectious Diseases (NIAID) Bethesda, US. One ng of supplied standard equals 39 units of Gxg01-902-535 NIAID-standard. Please note that the calibration is batch specific.

## Precision

Sample	Intra-assay			Inter-assay		
	1	2	3	1	2	3
n	10	10	10	3	3	3
Mean (pg/ml)	105.1	41.0	16.1	97.3	39.0	15.2
SD	4.2	1.9	1.0	7.8	2.3	1.1
CV (%)	4.0	4.7	6.2	8.0	5.9	7.2

Intra-assay and inter-assay precision were determined at 3 different concentrations of analyte (10 replicates per concentration in 3 assays).

### Recovery

	Spike concentration (pg/ml)	Average recovery (%)
Plasma pool	100	110
	40	102
	16	110
RF positive control plasma	100	81
	40	83
	16	86

Standard was spiked in a plasma pool from normal blood donors (5 replicates per concentration in 3 assays) or in an RF positive control plasma (1900 IU/ml RF, 3 replicates per concentration in two assays). Average recovery is listed.

### Linearity

Plasma samples were spiked with a high concentration of standard and diluted (1:2 to 1:8) in RF-block diluent. Recovery in a plasma pool from normal blood donors ranged from 97 to 114%. Recovery in RF positive control plasma ranged from 75 to 91%.

### Specificity

The kit is based on a matched pair of mAbs specific for native and recombinant human IFN- $\gamma$ .

Developed and manufactured by MABTECH AB, Sweden, whose quality management system complies with the standards ISO 9001:2015 & ISO 13485:2016.



**The products are for research use only.**

MABTECH shall not be liable for the use or handling of the product or for consequential, special, indirect or incidental damages there from.

**Mabtech AB (Head Office)**  
Sweden  
Tel: +46 8 716 27 00  
mabtech@mabtech.com

**Mabtech, Inc.**  
USA  
Tel: +1 513 871-4500  
mabtech.usa@mabtech.com