Mouse IgA
ELISA development kit

Product Code: 3865-1AD-6

CONTENTS: development kit for 6 plates

Vial 1 (blue top)
Monoclonal MT45A antibody (300 µl)
Concentration: 0.5 mg/ml

Vial 2 (red top)
ALP-conjugated MT39A (80 µl)

Vial 3
Lyophilised mouse IgA standard

To ensure total recovery of stated quantity, vials have been overfilled.

STORAGE:
Shipped at ambient temperature. On arrival box 1 should be stored refrigerated at 4-8°C and box 2 should be stored frozen at -20°C.

General

Intended use: For quantitative determination of native mouse IgA in serum and plasma.

Reagents: MT45A is supplied in sterile-filtered (0.2 µm) PBS with sodium azide (0.02%). MT39A-ALP is supplied in 0.1 M Tris-buffer with 0.002% Kathon CG.

Recommended standard dilution: 0.1-100 ng/ml

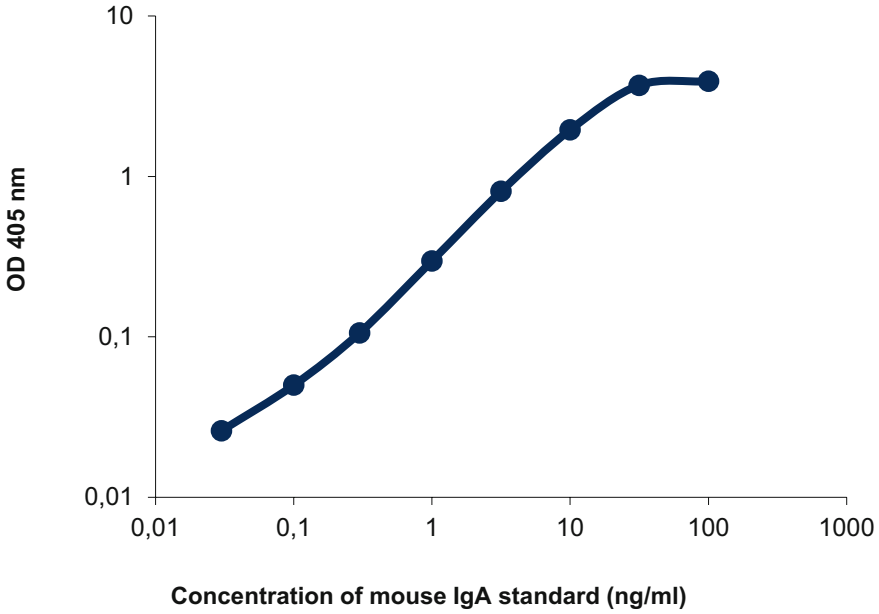

Guidelines for Mouse IgA ELISA

Day 1 1. Coat a high protein binding ELISA plate with mAb MT45A, diluted to 2 µg/ml in PBS, pH 7.4, by adding 100 µl/well. Incubate overnight at 4-8°C.

Day 2 2. Wash twice with PBS (200 µl/well).

3. Block plate by adding 200 µl/well of PBS with 0.05% Tween 20 (PBS-Tween) containing 0.1% BSA (incubation buffer*). Incubate for 1 hour at room temperature.

4. Wash five times with PBS-Tween.

5. Prepare mouse IgA standard by reconstituting contents of vial 3 in 500 µl PBS to make up a stock solution of 50 µg/ml. The stock solution should be used immediately or stored in aliquots at -20°C for future use. We recommend the aliquots not be refrozen after initial use. For the test, prepare dilutions of the stock using the standard range as a guideline.

6. Add 100 µl/well of samples or standards diluted in incubation buffer and incubate for 2 hours at room temperature.

7. Wash as in step 4.

8. Add 100 µl/well of MT39A-ALP diluted 1:1000 in incubation buffer. Incubate for 1 hour at room temperature.

9. Wash as in step 4.

10. Add 100 µl/well of appropriate substrate solution e.g. p-nitrophenyl-phosphate (pNPP).

11. Measure the optical density (405 nm for pNPP) in an ELISA reader after suitable developing time.

* The same buffer is used for blocking and for dilution.

MABTECH

Capture | Detect | Discover

Updated on 2020/03/31

Developed and manufactured by MABTECH AB, Sweden, whose quality management system complies with the standards ISO 9001:2015 & ISO 13485:2016.

SP CERTIFIED ISO 9001 Quality management systems RI.SE

SP CERTIFIED ISO 13485 Medical devices Quality management systems RI.SE

The products are for research use only.

MABTECH shall not be liable for the use or handling of the product or for consequential, special, indirect or incidental damages there from.

Mabtech AB (Head Office)
Sweden
Tel: +46 8 716 27 00
mabtech@mabtech.com

Mabtech, Inc.
USA
Tel: +1 513 871-4500
mabtech.usa@mabtech.com

www.mabtech.com